


**3 months later**

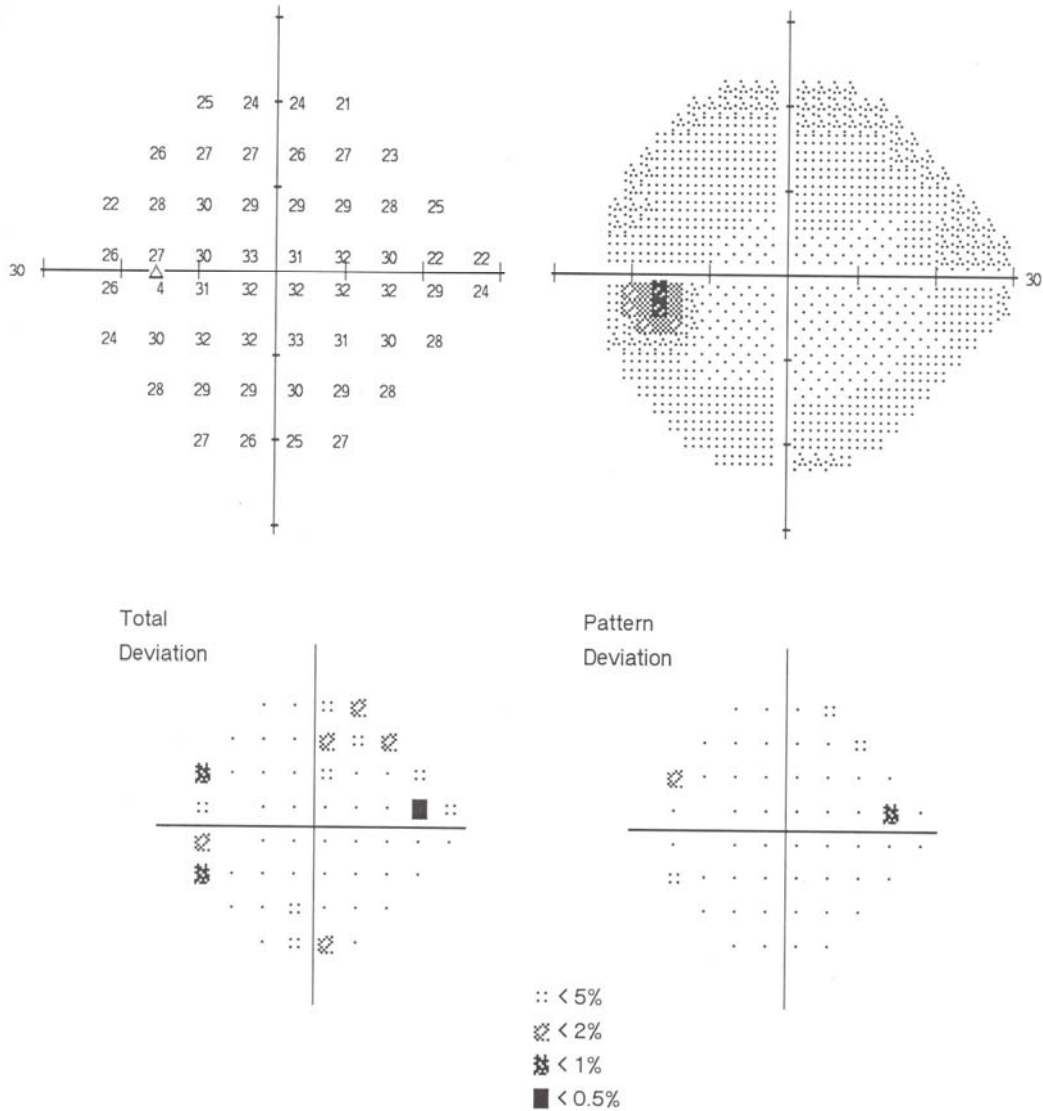

**Supplementary Figure S7.** The HVF results from 3 months after the initial testing for patient MS1. SITA standard central 24-2 threshold test was used. The mean deviation(MD) was improved to -2.60 dB (within normal limits) 3 months later.