


### 8 months later

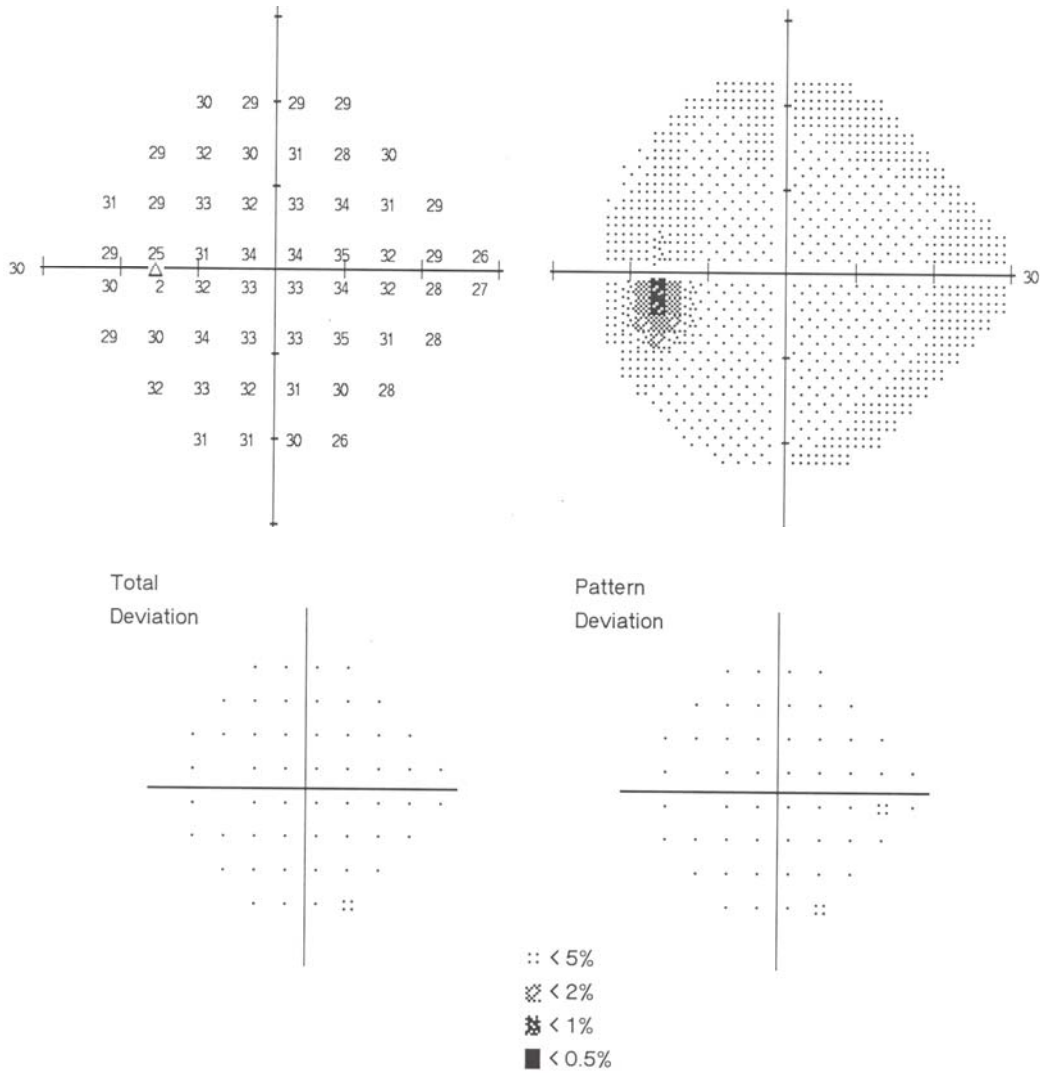

**Supplementary Figure S8.** The HVF results from 8 months after the initial testing for patient MS2. SITA standard central 24-2 threshold test was used. The MD was improved to - 0.44 dB (within normal limits) 8 months later.