


Supplementary Figure 1

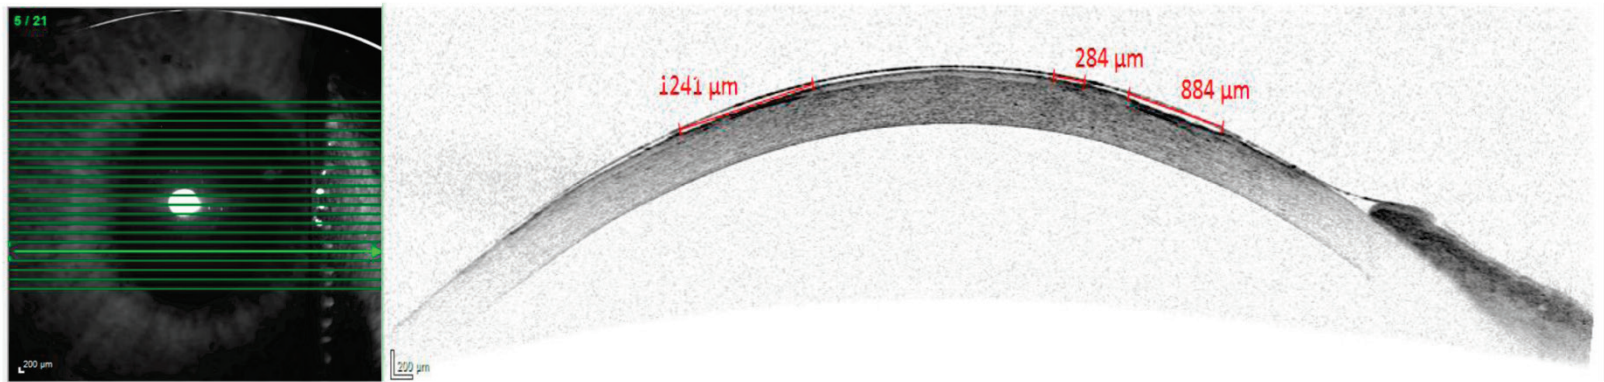

Supplementary Figure 1. Demonstration of the measurement of SD-OCT corneal erosions. The length of epithelial erosions (LED) in each B-scan was measured using the Spectralis OCT software (red marks).